


DETECT CELLS OR PARTICLES

«*Detect Cells or Particles*»

The pipeline purpose is to detect objects having a quite limited, well defined, structure. It can be applied to Cells, Nuclei or any kind of small particles

Arivis Vision4D Pipeline example «*Detect Cells or Particles*» Working Flowchart :

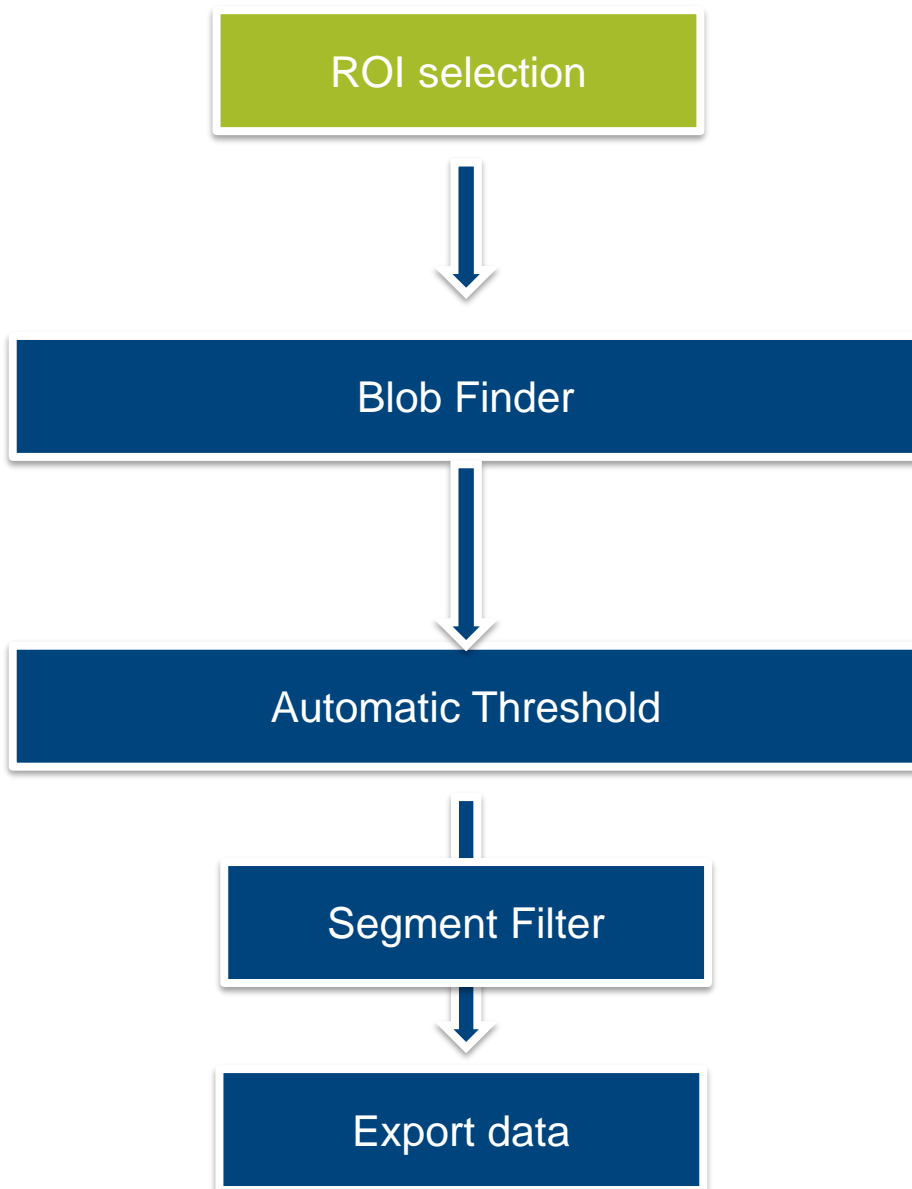

Arivis Vision4D Pipeline example

In order to run the pipeline described here below, please download the demo dataset according to the following instruction.


Step 1.

Click on the below link to access to the Arivis downloading demo dataset's area.



[Demo Dataset](#)

arivisVision4D-DemoData-SamplePipelines-DetectStructures.zip file is saved on the download folder.

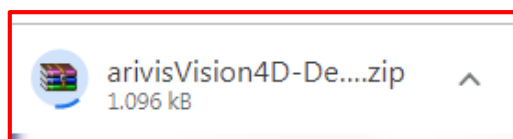


Step 2.

Create a new folder on your local disk.
Move the ZIP file from the download folder inside it.

Step 3.




UnZip the file:

arivisVision4D-DemoData-SamplePipelines-DetectStructures.zip.



Three files are now available in the folder.




	4Channels_3DStack.metadata	06/12/2018 10:12	File METADATA	4 KB
	4Channels_3DStack.objects	06/12/2018 10:12	File OBJECTS	108 KB
	4Channels_3DStack	06/12/2018 10:12	arivis SIS file	4,190 KB

Step 4.

Open the SIS file on Vision4D.


	4Channels_3DStack	06/12/2018 10:12	arivis SIS file	4,190 KB
---	-------------------	------------------	-----------------	----------

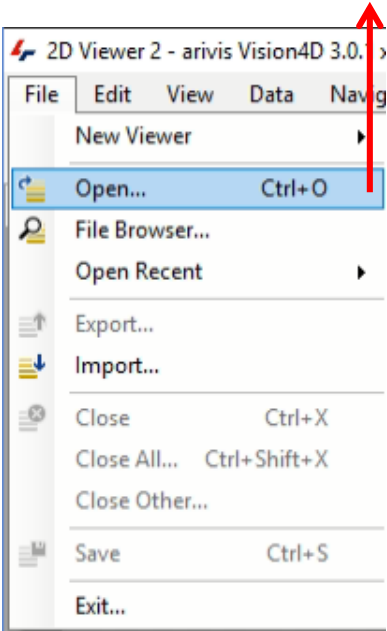

The dataset is visualized in the V4D viewing area.

TIPS :

The dataset is visualized according to the current rendering setting parameters. Please refer to the *User Manual* for more details about how to set or modify the rendering options.

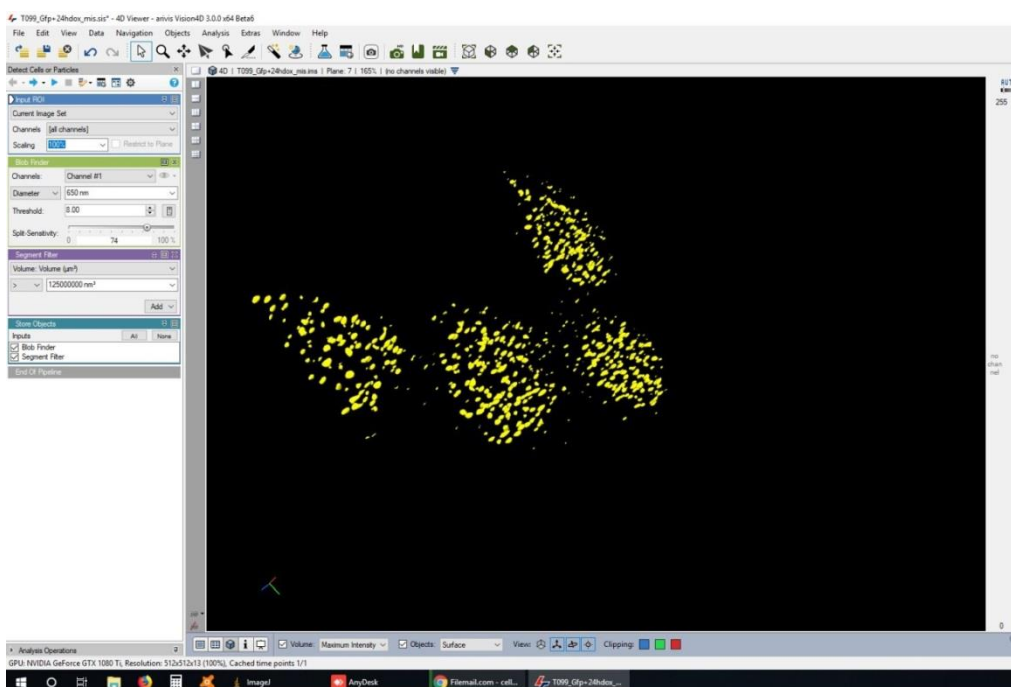


DETAILS:


The dataset is a multi dimensional, discrete, representation of your real sample volume. It can be structured as a Z series of planes (eg Optical sectioning) of multiple channels (dyes) in a temporal sequence of time points (located in several spatial positions). Usually the dataset shows a single experimental situation (a complete experiment can be composed by several datasets). The datasets are available as graphic files saved in plenty of graphic formats (standard cached formats as well as proprietary formats)

Step 4.

Activate the «*Detect Cells or Particles*» pipeline.

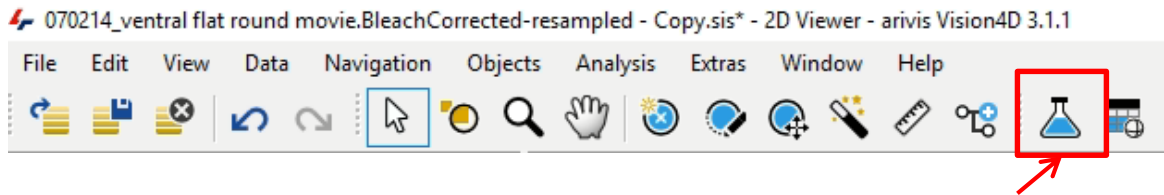

If not already done, open the Analysis panel

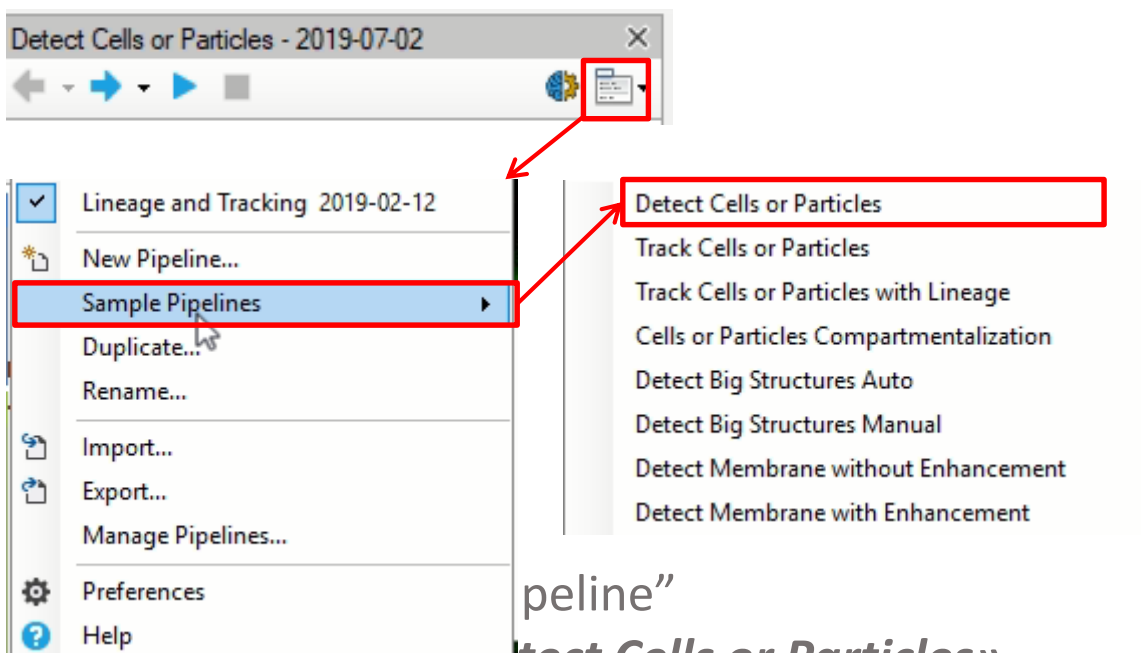


Then click on the «*Detect Cells or Particles*» item.

TIPS:

The active Pipeline, if any, will be replaced by the new one. Please refer to the **User Manual** for more details about how to export a pipeline.

The «*Detect Cells or Particles*» pipeline operators layout.

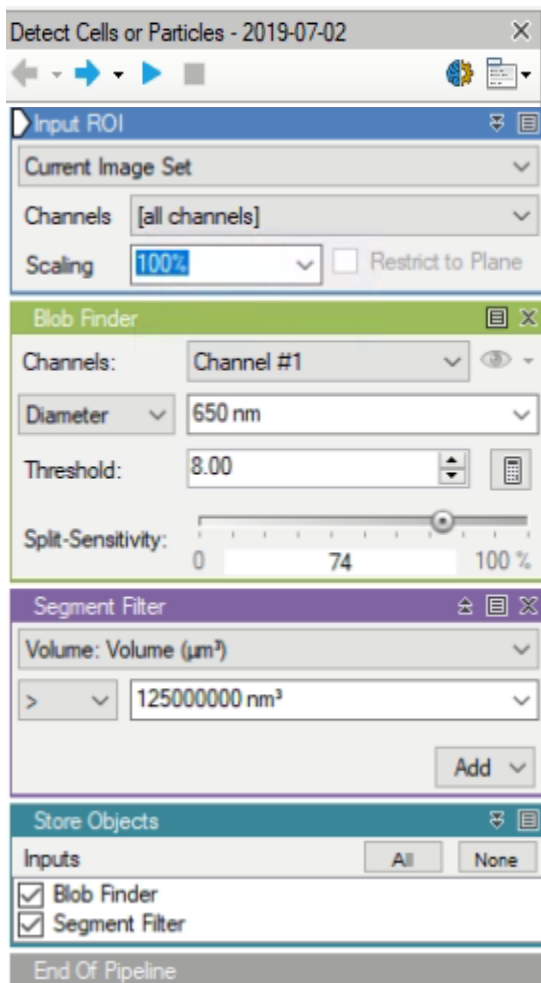

1. Region Of Interest:
This operator allows the region of interest (ROI) selection. ROI defines the dataset subarea that will be processed and analyzed by the pipeline.
2. Blobs Finder:
Automatic small objects detection algorithm. It uses a local threshold method.
3. Segment Filter
Allows the blob filtering based on multiple parameters selection.
4. Store Objects
Store the detected segments (TAG) in the active dataset.

Step 5.

Execute the «**Detect Cells or Particles**» pipeline.





TIPS :

The pipeline can be executed as single shot or step by step.


Step by step method allows to run and undo a single **Operation**.

Single shot method runs all the pipeline in one task (no stop until the pipeline execution ends).

Either the arrow buttons or the **Operation** list can be used to run both methods.

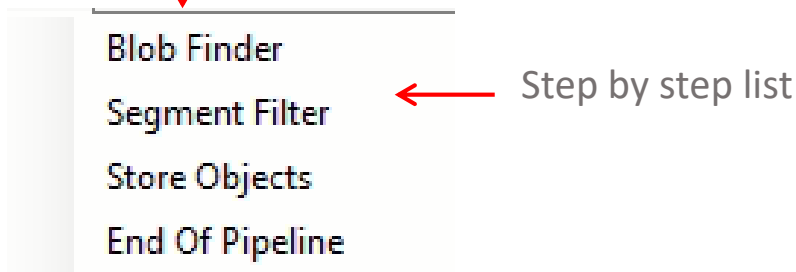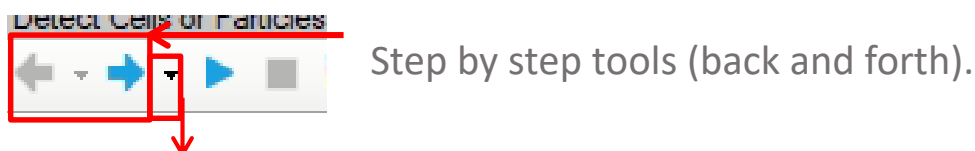

The white arrow on the operator title bar shows the next step that will be executed.




Step 6.


View the results

TIPS :

Results (segments and measurements) will be stored in the dataset only if the **Store Objects** operator has been correctly set. Please tick appropriately the option as shown below before complete the pipeline execution.

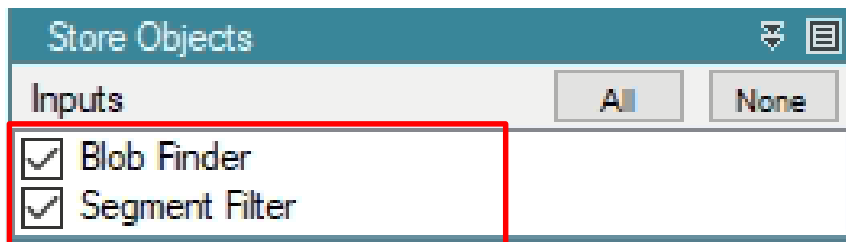

Measurements are now visible in the data table

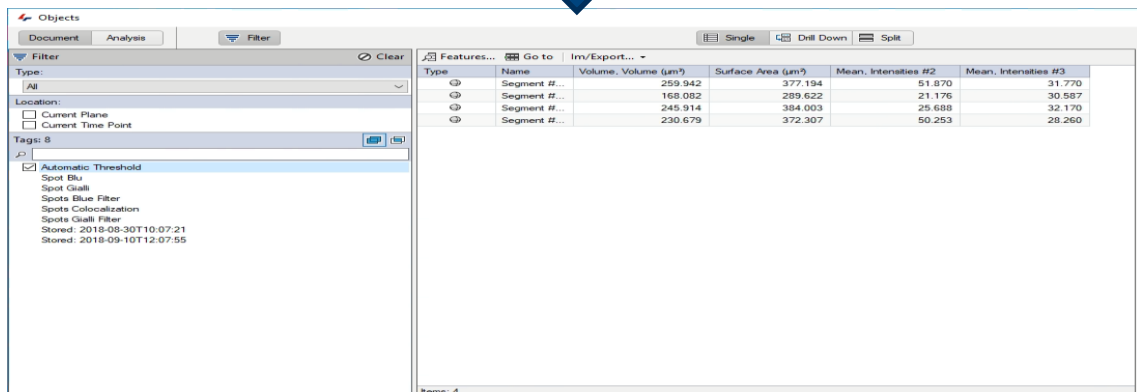

Type	Name	Volume, Volume (µm³)	Surface Area (µm²)	Mean, Intensities #2	Mean, Intensities #3
Segment #...		259.942	377.194	51.870	31.770
Segment #...		168.082	289.622	21.176	30.587
Segment #...		245.914	384.003	25.688	32.170
Segment #...		230.679	372.307	50.253	28.260


TIPS :

If the data table is not already visible, please click on the related icon to open it.



View the results.

Segments can be visualized either in 2D as well as 4D according to the currently set options.

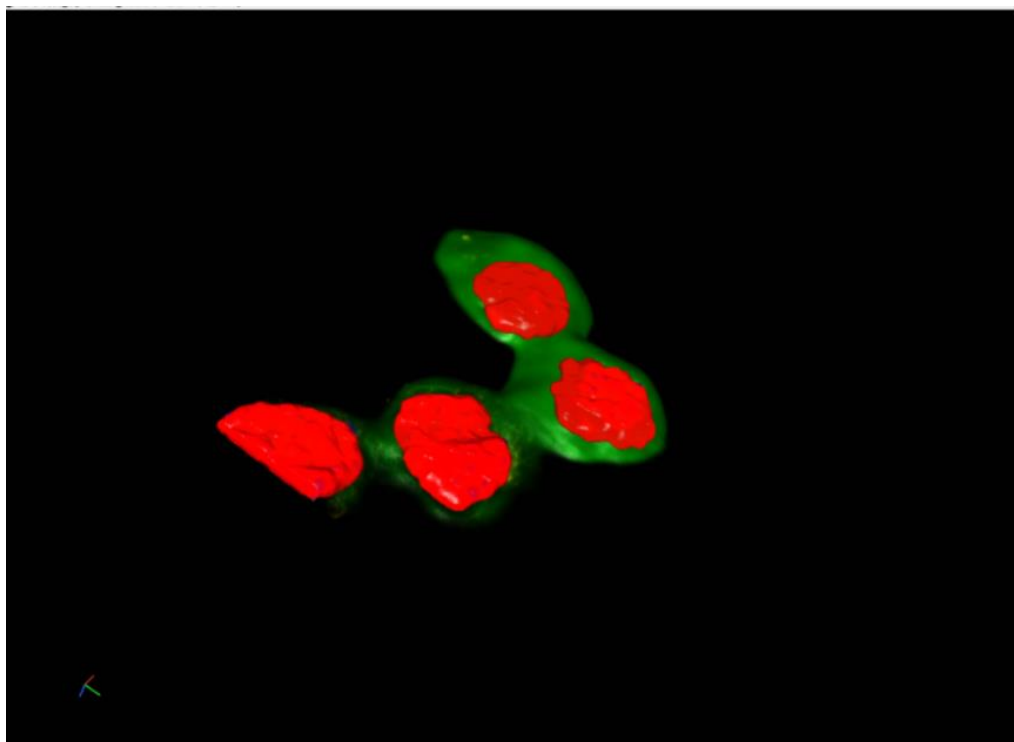

TIPS :

Please refer to the ***User Manual*** for more details about how to visualize segments on the dataset.

Arivis Vision4D Pipeline example

The «***Detect Cells or Particles***» pipeline can be modified to be adapted to your datasets.

All the pipeline parameters must be set according to your dataset features.

TIPS :

Before starting to modify the Pipeline layout, switch the Viewing area from 4D to 2D view mode.


During analysis setup, the Operator preview mode, is only available in 2D mode. Once the segments have been generated, you can switch back to 4D view mode.



TIPS :


Please refer to the ***User Manual*** for more details about how to switch the Viewing Area from 4D to 2D view mode.

Arivis Vision4D Pipeline setup

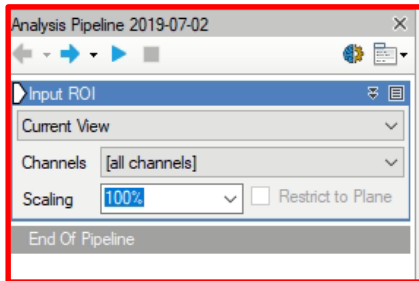

DETAILS:

The Analysis Pipeline panel consists of two main areas. The Pipeline sequence area and the analysis operations list area .

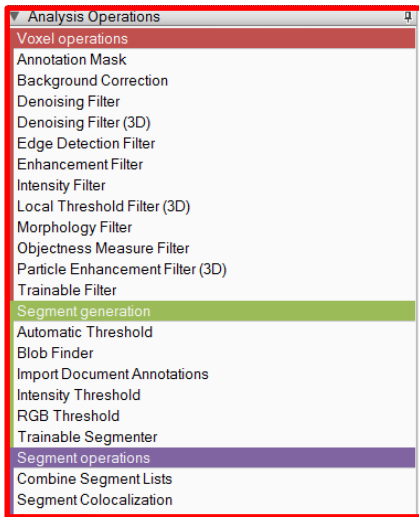

TIPS :

Please refer to [Addendum A](#) for more details about how to add or remove an **Operator** to the current Pipeline


DETAILS :

Analysis Pipeline protocol is executed from top to bottom of the pipeline. The Operations must be added to the Pipeline in the correct order.

Arivis Vision4D Pipeline setup

Step A.

How to set the **Input ROI** operator

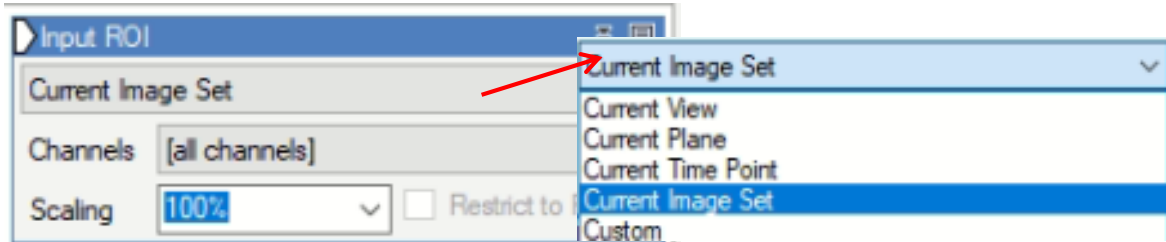

Processing & Analysis target options:

- a. Current View
Only the selected Z plane and the visualized area in the viewer are processed.
- b. Current Plane
Only the selected Z plane is processed regardless to the visualized area (real XY pixel size).
- c. Current Time Point
The selected time point is entirely processed (all Z planes and the real XY pixel size)
- d. Current Image Set
The complete dataset (XYZ and time) is processed.
- e. Custom
Allows a detailed selection of each parameters.

DETAILS :

Use the Custom option during the pipeline setting and testing . Set a sub volume (XY, Planes, Time Points, channels) of your dataset on which perform the trial. This will speedup the setting process.

TIPS :


Please refer to the **User Manual** for more details about how to select the active Z plane and/or the active Time Point.

Arivis Vision4D Pipeline setup

Step A

How to set the **Input ROI** operator Custom option

The full XY size, the viewing area or a free area setting (by coordinates) can be applied

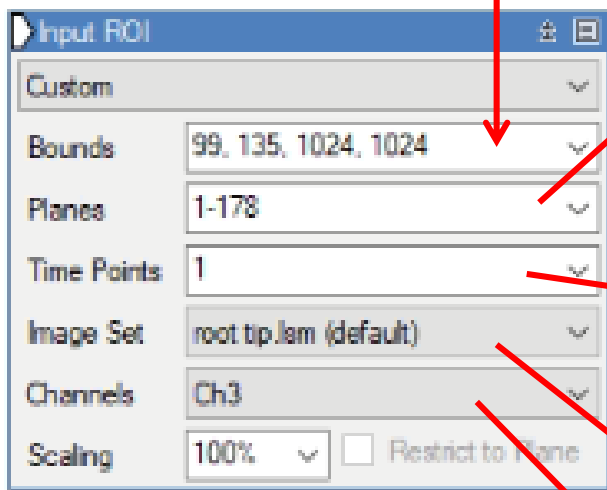

The screenshot shows the 'Input ROI' dialog box with the following settings:

- Custom** (selected in the dropdown)
- Bounds**: 99, 135, 1024, 1024
- Planes**: 1-178
- Time Points**: 1
- Image Set**: root.tip.lam (default)
- Channels**: Ch3
- Scaling**: 100% (dropdown), ☐ Restrict to Plane

Red arrows point from the following text blocks to the corresponding fields in the dialog box:


- Single Z plane, a range of Z planes or the full Z planes can be selected (points to the **Planes** field)
- Single Time point (TP), a range of TP or the full TP can be selected (points to the **Time Points** field)
- Select the source Image Set (points to the **Image Set** field)
- One or more of the available channels can be selected. Be careful, only the selected channel(s) can be used in the pipeline (points to the **Channels** field)
- The dataset volume can be downsized by 50 % or 25 %. This option is used to speed up analysis pipeline when the dataset is very large. (points to the **Scaling** section)

Arivis Vision4D Pipeline setup

Step B.

How to set the **Blob Finder** operator

Select working Channel(s).

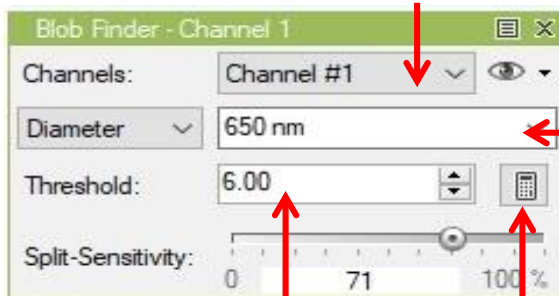

Set the reference objects diameter.

Set the object threshold coefficient.

Use the calculator to automatically set the threshold coefficient.




TIPS :

Object Diameter can be measured directly from the dataset.

Please refer to **Addendum B** for more details about how to measure object diameter.




Move the Split-Sensitivity slider to decrease/increase the splits objects sensitivity.

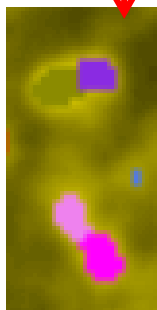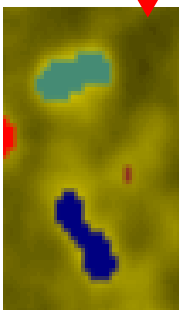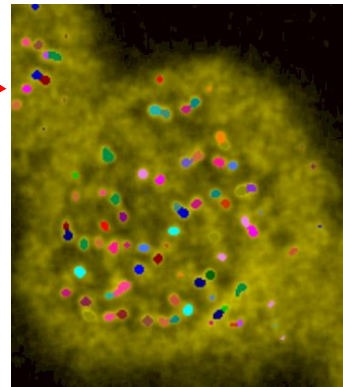

TIPS :


Use the *Navigator Panel* to select the preview Z plane and/or Time Points (if any)

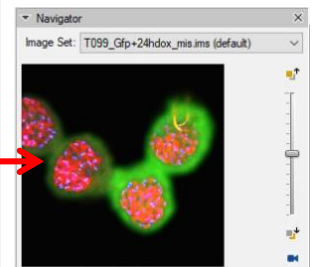

Arivis Vision4D Pipeline setup


Step C.

How to set the **Segment Filter** operator

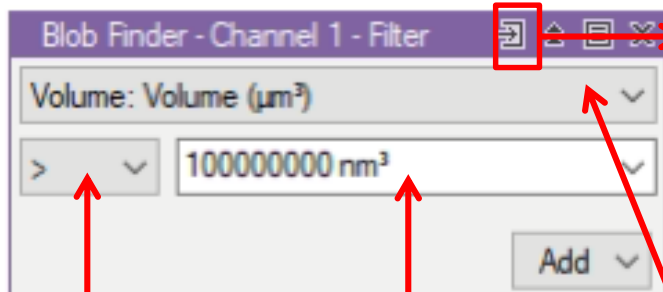


☒ Blob Finder - Channel 1
☐ Blob Finder - Channel 2

Select the Blob Finder operator source.

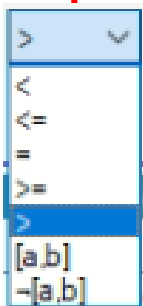

Set the limit used to filter the Blob Finder results according to the set filter rule. The values are expressed in metric unit


Select the filter rule.

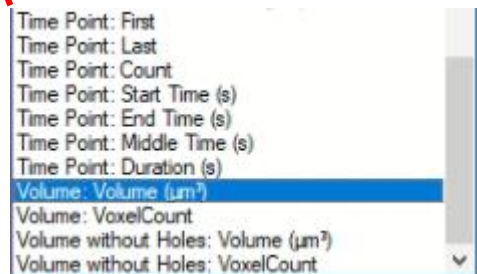

Select the Feature to be used for filtering the blobs

TIPS :

Segment Filter Tag can be renamed

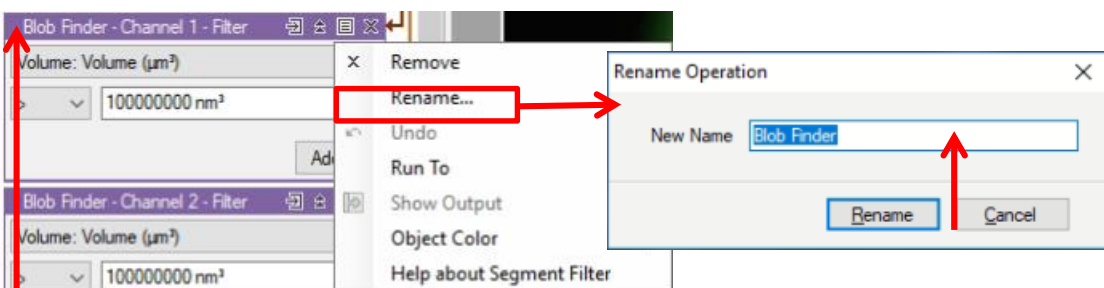



Right mouse click on the title bar

Digit the new Tag name and press **Rename**

Arivis Vision4D Pipeline setup

Addendum A:

How to add or remove an **Operator** from the pipeline.

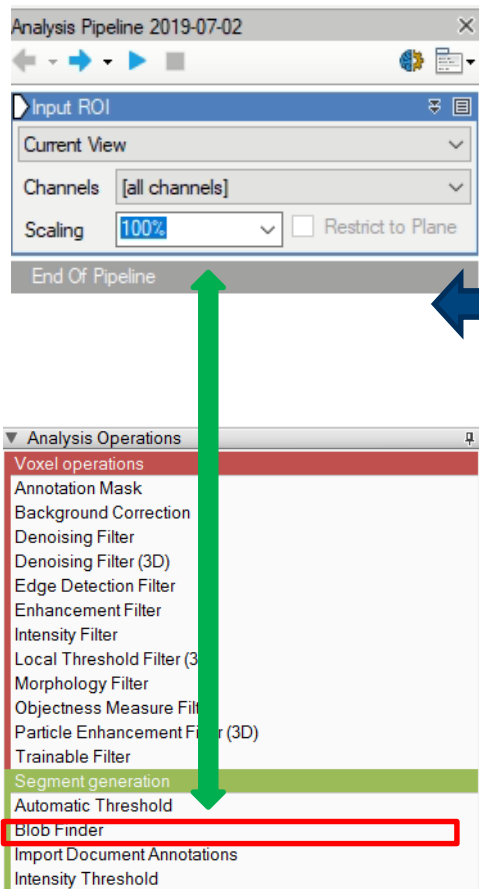

The **Operators** can be added to Pipeline in two ways

1. Double click on the **Operator** you wish to add to the current Pipeline.

The **Operator** will be inserted at the end of the group of operations to which it belongs. Voxel Operations are positioned before the Segment generation meanwhile Store operations are put always at the end of the Pipeline.

2. Drag and drop the **Operator** you wish to add to the current Pipeline.

The **Operator** will be automatically inserted in any place within the group of operations to which it belongs. The **Operator** cannot be added during the Pipeline execution

To remove an Operator from the Pipeline, press the X button located in the right side of the operator title bar.

TIPS :

Please refer to the **User Manual** for more details about how to add a new **Operator** to the current Pipeline.


Arivis Vision4D Pipeline setup

Addendum B:

How to measure Object diameter



Switch to 2D view mode.




Press the Ruler icon in the *Shortcut toolbar panel*.


1. Move the mouse cursor (it shows a little ruler instead of the standard arrow) on one side of the structure you want to measure.

2. Keeping the left mouse button down, draw a line over the structure diameter.

Once the mouse button is released, the distance measured is shown over the image.

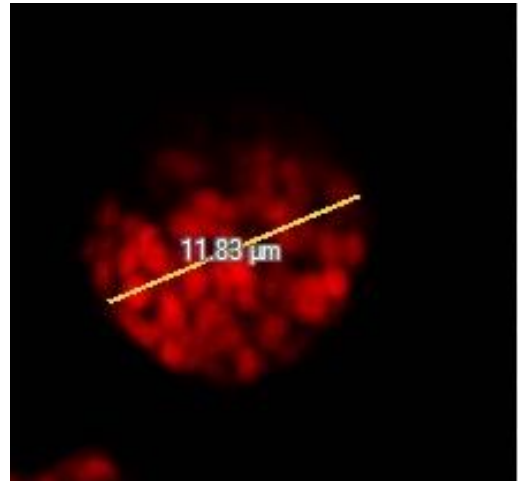

3. Take note of this number and digit it in the *Diameter Box*

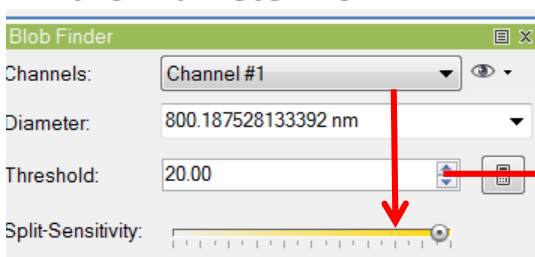

800.187528133392 nm

TIPS :

Before write down the diameter in the Box, select from the list the right metric unit you want to use.

Then digit the measure without delete the unit in the box